

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
21 April 2005 (21.04.2005)

PCT

(10) International Publication Number
WO 2005/034808 A1

(51) International Patent Classification⁷: **A61F 2/06**

(21) International Application Number:
PCT/US2004/033568

(22) International Filing Date: 12 October 2004 (12.10.2004)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/510,241 10 October 2003 (10.10.2003) US
60/529,346 12 December 2003 (12.12.2003) US

(71) Applicants (*for all designated States except US*):
WILLIAM A. COOK AUSTRALIA PTY. LTD.
[AU/AU]; 12 Electronics Street, Brisbane Technology
Park, Eight Mile Plains, Brisbane, QLD 4113 (AU).
COOK INCORPORATED [US/US]; 750 North Daniel's
Way, P.O. Box 489, Bloomington, IN 47402-0489 (US).

(72) Inventors; and


(75) Inventors/Applicants (*for US only*): **HARTLEY, David, Ernest** [AU/AU]; 2 View Street, Subiaco, W.A. 6008 (AU). **ANDERSON, John, Lennon** [AU/AU]; 96 Eve Road, Bellevue Heights, S.A. 5050 (AU). **LAWRENCE-BROWN, Michael** [AU/AU]; 77 Branksome Gardens, City Beach, W.A. 6015 (AU).

(74) Agent: **GODLEWSKI, Richard, J.**; P.O. Box 2269, Bloomington, IN 47402-2269 (US).

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM,

[Continued on next page]

(54) Title: FENESTRATED STENT GRAFTS

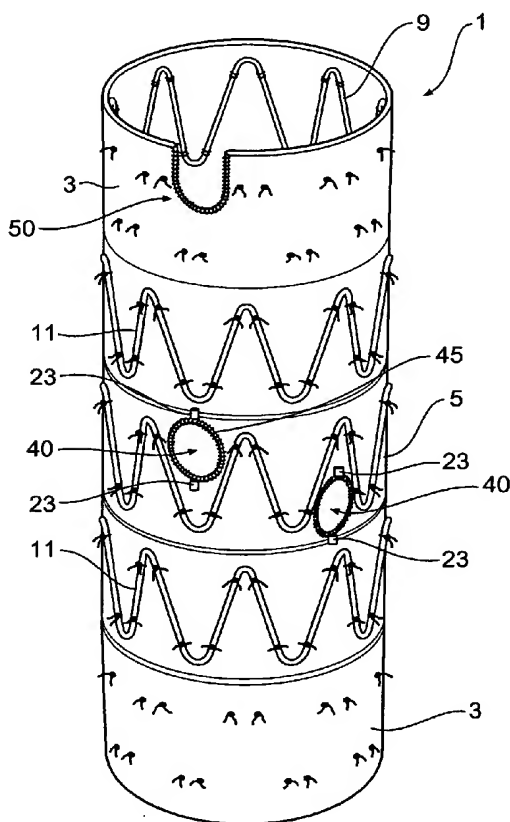

(57) Abstract: A stent graft (1) with at least one fenestration (40) including a peripheral (37) reinforcement around at least part of the fenestration. There can also be a tubular extension (15). The side arm includes a stent (19) and a cover (17) and extends from and is in fluid communication with the fenestration and the stent graft. The stent may be a self expanding stent. The ring and/or tubular extension provides better support and sealing for an extension arm. The fenestration (40) can be circular or if towards the ends of the stent graft may be in the form of a U-shape (50) with an open end.

WO 2005/034808 A1



TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI,

Published:

— *with international search report*

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

FENESTRATED STENT GRAFTS

DescriptionTechnical Field

This invention relates to a stent graft adapted for endovascular deployment and in particular to a fenestrated stent graft.

Background of the Invention

5 In our earlier patent application published as WO 99/29262 there was disclosed a stent graft including at least one fenestration to enable an extension leg graft to be extended from a main stent graft in an internal lumen through the fenestration to have the extension leg or arm graft extend into a branch vessel of the lumen. Such a situation may exist in the aorta with renal arteries extending
10 from the aorta. When there is an aneurism in this region which includes the junction of the aorta with the renal arteries then it is desirable to not only have a main graft which spans the aneurysm but also extension legs or arms which extend from the main graft into the renal or other arteries.

 A simple fenestration does not necessarily give a fully reliable support
15 and sealing surface for the extension leg graft and it is the object of this invention to improve the ability for support and sealing of an extension leg or arm grafts into a main graft.

Summary of the Invention

 The invention as claimed in Claim 1.

20 In one form, therefore, the invention is said to reside in a stent graft having a tubular wall and at least one fenestration in the tubular wall, the or each fenestration including a resilient material around at least a portion of the periphery thereof to provide dimensional stability to the fenestration.

 Preferably the resilient material may be selected from Nitinol™, stainless
25 steel or elastomeric material and may be in the form of a spring, expandable ring such as a slip ring or a portion of resilient wire.

 In one form the resilient material around the periphery may be in the form of a ring.

- 2 -

Preferably the ring includes at least two turns of wire and preferably the terminal ends of the wire of the ring are provided with a loop so that the wire does not present a pointed end of wire which could damage a vessel.

5 Alternatively, the ring may be a ring of a resilient material such as an elastomer. The elastomer may for instance be silicone elastomer.

Where the fenestration is adjacent an end of the stent graft the fenestration may be in the form of a scallop which is open at one side. The resilient material around the periphery may be in the form of a U-shape and during deployment may assist with opening up of the fenestration so that a vessel behind
10 the fenestration can be catheterized.

In another embodiment of a fenestration in the form of a scallop provided at the distal or proximal end of the stent graft may have struts of self expanding stents acting as resilient peripheral reinforcement around a portion of the fenestration. When the stent expands upon deployment, the struts spread apart
15 thereby opening up the fenestration.

The scallop may be at the proximal or distal end of a stent graft. For instance, when deploying a stent graft extending from the thoracic arch, a fenestration may be provided to prevent the coeliac artery being occluded. As with all embodiments, radiopaque or MRI opaque markers may be used to define the
20 periphery of the fenestration.

When deploying a stent graft into the lower aorta in the region of the aortic bifurcation, it may be desirable to provide a scalloped fenestration at the proximal end of the stent graft to avoid occluding the renal arteries or the superior mesenteric artery. Where these arteries are close together the scalloped
25 fenestration may be of such a size that it extends over more than one of the openings to the arteries.

The U-shape of resilient material can be a Nitinol™ on a stainless steel wire or may be a portion of an elastomeric material such as a silicone elastomer.

The fenestration may be surrounded by radiopaque markers to assist
30 with visualisation by suitable radiographic techniques. Alternatively there may be

- 3 -

included in or associated with the resilient material a gold or other heavy metal wire or band to provide the necessary visualisation.

In one embodiment the fenestration may include a tubular extension between the tubular wall and the ring.

5 The tubular extension may include a self expanding stent and an associated lining or covering of a biocompatible graft material.

10 In an alternative form the invention is said to reside in a stent graft having at least one fenestration, the or each fenestration including a tubular extension, the side arm including a stent and extending from and in fluid communication with the fenestration and the stent graft.

15 Preferably the tubular extension includes an associated lining or covering of a biocompatible graft material. By this arrangement the inner cylindrical surface of the tubular extension provides a larger support and sealing surface between fenestration in the main graft and an outer cylindrical surface of a side branch stent graft which has been deployed through the fenestration.

 Preferably the stent in the tubular extension is a self expanding stent which may be Nitinol™ or stainless steel. Alternatively the stent in the tubular extension may be a balloon expandable stent.

20 In one form the stent may be in the form of a Gianturco style zig zag Z stent. Alternatively the stent may be a Nitinol™ self expanding stent of the type known as a Zilver™ stent sold by Cook Incorporated.

 The bio-compatible graft material may be either on the inside or the outside of the stent or there may be a cover which extends over both the inside and the outside of the stent on the tubular extension.

25 There may be further included a ring of a resilient material around the periphery at the terminal end of the tubular extension to provide dimensional stability to the tubular extension to assist with sealing. The ring may be formed from one or more and preferably two or more circular turns of Nitinol™ or stainless steel wire and preferably have a loop at each of its ends to prevent the wire from
30 presenting a sharp end which might protrude through the graft material and pierce a lumen wall.

- 4 -

The bio-compatible material may be dacron, Thoralon™, expanded polytetrafluoroethylene or other synthetic bio-compatible material.

While Dacron, expanded polytetrafluoroethylene (ePTFE), or other synthetic biocompatible materials can be used to fabricate the coverings for the stent graft and the tubular extension, a naturally occurring biomaterial, such as collagen, is highly desirable, particularly a specially derived collagen material known as an extracellular matrix (ECM), such as small intestinal submucosa (SIS). Besides SIS, examples of ECM's include pericardium, stomach submucosa, liver basement membrane, urinary bladder submucosa, tissue mucosa, and dura mater.

SIS is particularly useful, and can be made in the fashion described in Badylak et al., US Patent 4,902,508; Intestinal Collagen Layer described in US Patent 5,733,337 to Carr and in 17 Nature Biotechnology 1083 (Nov. 1999); Cook et al., WIPO Publication WO 98/22158, dated 28 May 1998, which is the published application of PCT/US97/14855. Irrespective of the origin of the material (synthetic versus naturally occurring), the material can be made thicker by making multilaminate constructs, for example SIS constructs as described in US Patents 5,968,096; 5,955,110; 5,885,619; and 5,711,969. Animal data show that the SIS used in grafts can be replaced by native tissue in as little as a month's time. In addition to xenogenic biomaterials, such as SIS, autologous tissue can be harvested as well. Additionally Elastin or Elastin-Like Polypeptides (ELPs) and the like offer potential as a material to fabricate the graft to form a device with exceptional biocompatibility. Another alternative would be to use allografts such as harvested native tissue. Such tissue is commercially available in a cryopreserved state.

The tubular extension may be placed on a reduced diameter portion of the stent graft so that the overall diameter of the stent graft is not significantly affected.

For this specification the term 'tubular extension' in relation to the side arm, is intended to mean that the length of the tubular extension is substantially similar in order of magnitude to the diameter of the tubular extension. Hence for a tubular extension diameter of 6 millimetres the length may be in the range of 5

- 5 -

to 10 millimetres. Such a tubular extension diameter would be suitable for deploying an extension leg or arm graft for a renal artery extending from an aorta.

The stent graft may have a diameter of from 20 to 40 mm and a length of from 100 to 250 mm. The placement of the fenestrations and the tubular extensions where required is dependant upon the particular body lumen and each set of fenestrations would normally be custom designed. The main stent graft may include a proximally extending uncovered stent to assist with retention within a body lumen such as an aorta.

The main stent graft in which the fenestration is provided may be one of the components of a composite graft.

U.S. Patent No. 5,387,235 entitled "Expandable Transluminal Graft Prosthesis For Repair Of Aneurysm" discloses apparatus and methods of retaining grafts onto deployment devices. These features and other features disclosed in U.S. Patent No. 5,387,235 could be used with the present invention and the disclosure of U.S. Patent No. 5,387,235 is herewith incorporated in its entirety into this specification.

U.S. Patent No. 5,720,776 entitled "Barb and Expandable Transluminal Graft Prosthesis For Repair of Aneurysm" discloses improved barbs with various forms of mechanical attachment to a stent. These features and other features disclosed in U.S. Patent No. 5,720,776 could be used with the present invention and the disclosure of U.S. Patent No. 5,720,776 is herewith incorporated in its entirety into this specification.

U.S. Patent No. 6,206,931 entitled "Graft Prosthesis Materials" discloses graft prosthesis materials and a method for implanting, transplanting replacing and repairing a part of a patient and particularly the manufacture and use of a purified, collagen based matrix structure removed from a submucosa tissue source. These features and other features disclosed in U.S. Patent No. 6,206,931 could be used with the present invention and the disclosure of U.S. Patent No. 6,206,931 is herewith incorporated in its entirety into this specification.

PCT Patent Publication No. WO 98/53761 entitled "A Prosthesis And A Method And Means Of Deploying A Prosthesis" discloses an introducer for a

- 6 -

prosthesis which retains the prosthesis so that each end can be moved independently. These features and other features disclosed in PCT Patent Publication No. WO 98/53761 could be used with the present invention and the disclosure of PCT Patent Publication No. WO 98/53761 is herewith incorporated in its entirety into this specification.

U.S. Patent No. 6,524,335 and PCT Patent Publication No. WO 99/29262 entitled "Endoluminal Aortic Stents" disclose a fenestrated prosthesis for placement where there are intersecting arteries. This feature and other features disclosed in U.S. Patent No. 6,524,335 and PCT Patent Publication No. WO 99/29262 could be used with the present invention and the disclosure of U.S. Patent No. 6,524,335 and PCT Patent Publication No. WO 99/29262 is herewith incorporated in its entirety into this specification.

U.S. Patent Application Serial No. 10/280,486, filed October 25, 2002 and published on May 8, 2003 as U.S. Patent Application Publication No. US-2003-0088305-A1 and PCT Patent Publication No. WO 03/034948 entitled "Prostheses For Curved Lumens" discloses prostheses with arrangements for bending the prosthesis for placement into curved lumens. This feature and other features disclosed in U.S. Patent Application Serial No. 10/280,486, and U.S. Patent Application Publication No. US-2003-0088305-A1 and PCT Patent Publication No. WO 03/034948 could be used with the present invention and the disclosure of U.S. Patent Application Serial No. 10/280,486, and U.S. Patent Application Publication No. US-2003-0088305-A1 and PCT Patent Publication No. WO 03/034948 is herewith incorporated in its entirety into this specification.

U.S. Provisional Patent Application Serial No. 60/392,682, filed June 28, 2002, U.S. Patent Application Serial No. 10/447,406, filed May 29, 2003, and Published on December 18, 2003, as U.S. Patent Application Publication No. US-2003-0233140-A1, and PCT Patent Publication No. WO 03/101518 entitled "Trigger Wires" disclose release wire systems for the release of stent grafts retained on introducer devices. This feature and other features disclosed in U.S. Provisional Patent Application Serial No. 60/392,682, U.S. Patent Application Serial No. 10/447,406, and U.S. Patent Application Publication No. US-2003-0233140-A1, and

- 7 -

PCT Patent Publication No. WO 03/101518 could be used with the present invention and the disclosure of U.S. Provisional Patent Application Serial No. 60/392,682, U.S. Patent Application Serial No. 10/447,406, and U.S. Patent Application Publication No. US-2003-0233140-A1, and PCT Patent Publication No. WO 03/101518 is herewith incorporated in its entirety into this specification.

U.S. Provisional Patent Application Serial No. 60/392,667, filed June 28, 2002, and U.S. Patent Application Serial No. 10/609,846, filed June 30, 2003, and Published on May 20, 2004, as US Patent Application Publication No. US-2004-0098079-A1, and PCT Patent Publication No. WO 2004/028399 entitled "Thoracic Deployment Device" disclose introducer devices adapted for deployment of stent grafts particularly in the thoracic arch. This feature and other features disclosed in U.S. Provisional Patent Application Serial No. 60/392,667, U.S. Patent Application Serial No. 10/609,846, and US Patent Application Publication No. US-2004-0098079-A1, and PCT Patent Publication No. WO 2004/028399 could be used with the present invention and the disclosure of U.S. Provisional Patent Application Serial No. 60/392,667, U.S. Patent Application Serial No. 10/609,846, and US Patent Application Publication No. US-2004-0098079-A1, and PCT Patent Publication No. WO 2004/028399 is herewith incorporated in its entirety into this specification.

U.S. Provisional Patent Application Serial No. 60/392,599, filed June 28, 2002, and U.S. Patent Application Serial No. 10/609,835, filed June 30, 2003, and published on June 3, 2004, as U.S. Patent Application Publication No. US-2004-0106978-A1, and PCT Patent Publication No. WO 2004/002370 entitled "Thoracic Aortic Aneurysm Stent Graft" disclose stent grafts that are useful in treating aortic aneurysms particularly in the thoracic arch. This feature and other features disclosed in U.S. Provisional Patent Application Serial No 60/392,599, U.S. Patent Application Serial No. 10/609,835, and U.S. Patent Application Publication No. US-2004-0106978-A1, and PCT Patent Publication No. WO 2004/002370 could be used with the present invention, and the disclosure of U.S. Provisional Patent Application Serial No 60/392,599, U.S. Patent Application Serial No. 10/609,835, and U.S. Patent Application Publication No. US-2004-0106978-A1, and PCT Patent

- 8 -

Publication No. WO 2004/002370 is herewith incorporated in its entirety into this specification.

U.S. Provisional Patent Application Serial No. 60/391,737, filed June 26, 2002, U.S. Patent Application Serial No. 10/602,930, filed June 24, 2003, and PCT Patent Publication Number WO 2004/002365 entitled "Stent-Graft Fastening" disclose arrangements for fastening stents onto grafts particularly for exposed stents. This feature and other features disclosed in U.S. Provisional Patent Application No. 60/391,737, U.S. Patent Application Serial No. 10/602,930, and PCT Patent Publication Number WO 2004/002365 could be used with the present invention and the disclosure of U.S. Provisional Patent Application Serial No. 60/391,73, U.S. Patent Application Serial No. 10/602,930, and PCT Patent Publication Number WO 2004/002365 are herewith incorporated in its entirety into this specification.

U.S. Provisional Patent Application Serial No. 60/405,367, filed August 23, 2002, U.S. Patent Application Serial No. 10/647,642, filed August 25, 2003, and PCT Patent Publication No. WO 2004/017868 entitled "Asymmetric Stent Graft Attachment" disclose retention arrangements for retaining onto and releasing prostheses from introducer devices. This feature and other features disclosed in U.S. Provisional Patent Application Serial No. 60/405,367, filed August 23, 2002, U.S. Patent Application Serial No. 10/647,642, filed August 25, 2003, and PCT Patent Publication No. WO 2004/017868 could be used with the present invention and the disclosure of U.S. Provisional Patent Application Serial No. 60/405,367, filed August 23, 2002, U.S. Patent Application Serial No. 10/647,642, filed August 25, 2003, and PCT Patent Publication No. WO 2004/017868 are herewith incorporated in its entirety into this specification.

U.S. Patent Application Serial No. 10/322,862, filed December 18, 2002 and published as Publication No. US2003-0120332, and PCT Patent Publication No. WO03/053287 entitled "Stent Graft With Improved Adhesion" disclose arrangements on stent grafts for enhancing the adhesion of such stent grafts into walls of vessels in which they are deployed. This feature and other features disclosed in U.S. Patent Application Serial No. 10/322,862, filed December 18, 2002 and published as

- 9 -

Publication No. US2003-0120332, and PCT Patent Publication No. WO03/053287 could be used with the present invention and the disclosure of U.S. Patent Application Serial No. 10/322,862, filed December 18, 2002 and published as Publication No. US2003-0120332, and PCT Patent Publication No. WO03/053287 are herewith incorporated in its entirety into this specification.

U.S. Provisional Patent Application Serial No. 60/405,769, filed August 23, 2002, U.S. Patent Application Serial No. 10/645,095, filed August 23, 2003, and PCT Patent Publication Number WO 2004/017867 entitled "Composite Prostheses" discloses prostheses or stent grafts suitable for endoluminal deployment. These prostheses and other features disclosed in U.S. Provisional Patent Application Serial No. 60/405,769, filed August 23, 2002, U.S. Patent Application Serial No. 10/645,095, filed August 23, 2003, and PCT Patent Publication Number WO 2004/017867, could be used with the present invention and the disclosure of U.S. Provisional Patent Application Serial No. 60/405,769, filed August 23, 2002, U.S. Patent Application Serial No. 10/645,095, filed August 23, 2003, and PCT Patent Publication Number WO 2004/017867 are herewith incorporated in its entirety into this specification.

Brief Description of the Drawing

This then generally describes the invention but to assist with understanding reference will now be made to the accompanying drawings which show a preferred embodiment of the invention.

In the drawings:

Figure 1 shows one embodiment of a stent graft according to this invention;

Figure 2 shows a cross section of the stent graft shown in Figure 1 along the line 2 - 2';

Figure 3 shows a cross section through a tubular extension in one embodiment of the invention;

Figure 4 shows a part cut away view of the embodiment shown in Figure 3;

Figure 5 shows an alternative embodiment of a stent graft according to this invention;

- 10 -

Figure 6 shows a cross section through a fenestration shown in Figure 5;

Figure 7 shows a part cut away view of a fenestration of the embodiment shown in Figure 5;

5 Figure 8 shows a detailed view of the inside of a scalloped fenestration according to one embodiment of the invention;

Figure 9 shows an inside view of the embodiments shown in Figure 8;

Figure 10 shows an alternative embodiment of fenestration with a resilient elastomer ring surrounding the periphery of the fenestration;

Figure 11 shows another view of the embodiment of Figure 10;

10 Figure 12 shows an alternative embodiment of a stent graft with a scalloped fenestration;

Figure 13 shows a detailed internal view of the scalloped fenestration of Figure 12;

15 Figure 13A shows an internal view of an alternative arrangement of a scalloped fenestration;

Figure 14 shows an alternative embodiment of a stent graft with a scalloped fenestration; and

Figure 15 shows a detailed internal view of the scalloped fenestration of Figure 14.

20 Detailed Description

Now looking more closely at the drawings and in particular the embodiment shown in Figures 1 and 2 it will be seen that a main stent graft 1 comprises a tubular body portion 3 at proximal and distal ends of the stent graft 1 with a central reduced diameter portion 5 between the ends of the stent graft with tapered portions 6 and 7 extending from the tubular body portions 3 at each end to the central reduced diameter portion 5.

30 All of the tubular body portions, the tapered portions and the central portion are a biocompatible graft material such as Dacron, Thoralon™, expanded PTFE or a naturally occurring biomaterial, such as an extracellular matrix, such as small intestinal submucosa or other suitable material or a combination of these materials.

Gianturco style zig zag Z stents 9 are provided inside the graft material of the

- 11 -

tubular body portions 3 at each end and in between the ends Gianturco zig zag style Z stents 11 are provided on the tapering portions 6 and 7 and on the reduced diameter portion 5 outside of the graft material. There may be further Gianturco style zig zag Z stents on each of the tubular body portions 3, the tapering portions 6 and 7 and the reduced diameter portion 5 depending upon the overall length of the stent graft 1.

In the reduced diameter central portion 5 there is at least one substantially circular fenestration or aperture 13 on the tubular wall of the stent graft. In this embodiment there are three fenestrations being one for each of the two renal arteries and one for the superior mesenteric artery. Other numbers of fenestrations may also be used. The fenestrations 13 are substantially circular and extending from the fenestrations are tubular extensions 15. The tubular extensions 15 comprise a bio-compatible material tube 17 with a self expanding stent 19. In this embodiment the self expanding stent 19 is provided on the outer surface of the tubular extension but in an alternative embodiment the self expanding stent 19 may be provided on the inner surface of the graft material 17.

The biocompatible material tube 15 is a biocompatible graft material such as Dacron, Thoralon™, expanded PTFE or a naturally occurring biomaterial, such as an extracellular matrix, such as small intestinal submucosa or other suitable material.

Stitching 21 is provided to retain the tubular extension to the main graft.

Radiopaque markers 23 are provided at each end of the fenestration 13 at the base of the tubular extension 15 to assist a physician to locate the fenestration in respect to a side vessel extending from a main vessel. The radiopaque markers 23 may be gold or other convenient material.

In the embodiment shown in Figures 3 and 4 the tubular extension generally shown as 30 extends from a fenestration or aperture 31 in the side wall of a main stent graft 32. The tubular extension 30 includes a self expanding Nitinol™ stent 34 with a bio-compatible graft material inner layer 35 and outer layer 36. A ring 37 of Nitinol™ around the periphery of the tubular extension at the terminal end 39 is provided to give good dimensional stability to the distal end of the tubular

- 12 -

extension 30. In an alternative arrangement the ring 37 may be formed from stainless steel or any other convenient material. Stitching 41 is provided to retain the tubular extension to the main graft and stitching 42 is used to retain the ring 37 at the terminal end 39 of the tubular extension 30.

5 The ring 37 of Nitinol™ comprises two turns of wire with a loop 38 at each end of the wire. The loops 38 are provided to prevent the chance of damage to lumen wall because the pointed end of the wire is effectively enclosed within the loop.

10 It will be seen that by these various embodiments of this form of the invention that the tubular extension provides a good support and sealing surface into which another bio-compatible material stent graft may be deployed to extend into a branch artery from a main artery or other lumen of the body.

15 Figures 5 to 7 show an alternative embodiment of a stent graft according to this invention. In this embodiment the same reference numerals as used in Figure 1 are used for corresponding components.

 A main stent graft 1 comprises a tubular body portion 3 at proximal and distal ends of the stent graft 1 with a central tubular body portion 5.

20 All of the tubular body portions are a biocompatible graft material such as Dacron, Thoralon™, expanded PTFE or a naturally occurring biomaterial, such as an extracellular matrix, such as small intestinal submucosa or other suitable material.

25 Gianturco style zig zag Z stents 9 are provided inside the graft material of the tubular body portions 3 at each end and on the central tubular body portion 5. Gianturco style zig zag Z stents 11 are provided on the outside of the graft material. There may be further Gianturco style zig zag Z stents on each of the tubular body portions 3 and the central tubular portion 5 than those illustrated depending upon the overall length of the stent graft 1.

30 In the central tubular body portion 5 there is at least one substantially circular fenestration or aperture 40 on the tubular wall of the stent graft. In this embodiment there are two fenestrations being one for each of the two renal arteries when this embodiment is deployed into the aorta. Other numbers of fenestrations

- 13 -

may also be used where the placement of the stent graft involves the possibility of occluding other branch vessels such as the superior mesenteric artery. The fenestrations 40 are substantially circular. Radiopaque markers 23 are provided at each end of the fenestration 40 to assist a physician to locate the fenestration 40 in respect to a side vessel extending from a main vessel. The radiopaque markers 23 may be gold or other convenient material.

A ring 45 of Nitinol™ as can particularly be seen in Figures 6 and 7 is provided around the periphery of the fenestration 40 to give good dimensional stability to the fenestration 40. In an alternative arrangement the ring 45 may be formed from stainless steel or any other convenient material. Stitching 47 is provided to retain the ring 45 around the periphery of the fenestration 40.

The ring 45 of Nitinol™ preferably comprises at least two turns of wire with a loop 49 at each end of the wire. The loops 49 are provided to prevent the chance of damage to lumen wall because the pointed ends of the wire are effectively enclosed within the respective loops.

Alternatively one of the wires 45 may be a gold or other biocompatible heavy metal wire to provide radiographic visualisation of the ring to assist with positioning of the graft with respect to the branch vessel.

Also in Figure 5 there is shown a scalloped fenestration 50 which opens to the end 52 of the stent graft. Detail of the scalloped fenestration 50 can be seen in Figures 8 and 9.

Figure 8 shows an external view of a scalloped fenestration which can be placed at either the distal or proximal end of a stent graft and Figure 9 shows an internal view of the fenestration shown in Figure 8. The fenestration comprises a scallop of graft material cut out of the body of the graft 3. As can be seen in Figure 9 an arch of resilient wire 52 is stitched around the periphery 54 of the scalloped fenestration. The wire 52 has a loop 56 formed at each end of it so that no sharp end of the wire is provided which could damage the wall of a vessel into which the stent graft is deployed. Because the wire or other material from which the U-shaped reinforcement 52 is resilient the fenestration will close up when the stent graft is in a contracted state for deployment into a bodily lumen such as the aorta and when

- 14 -

released will open up to enable blood flow through the fenestration to a branch vessel.

The arch of resilient wire 52 is preferably made from a number of strands, such as three strands, of a resilient wire such as Nitinol™. The wire is stitched to the periphery of the fenestration with stitches 53.

Figures 10 and 11 show two views of an alternative fenestration arrangement according to the invention. In this embodiment the fenestration 60 is provided in the wall 5 of a stent graft and surrounding the fenestration 60 and providing reinforcement is an elastomeric ring 62 of a material such as silicon elastomer. The elastomeric ring 62 is sewn by stitching 64 into the periphery of the fenestration 60. Once again the elastomeric ring can be deformed so that it can be deployed within a deployment device and will open into the shape of the fenestration when deployed. The elastomeric ring will provide a certain amount of resiliency in position of the fenestration over a branch vessel and if deploying a side arm through the fenestration the elastomeric ring will provide a degree of blood sealing onto the branch stent graft.

Figures 12 and 13 show an alternative arrangement of fenestration on a stent graft. In Figure 12 the stent graft 68 comprises a tubular body of graft material 70 with a lumen therethrough. The distal end 72 of the stent graft has distally extending exposed stent 74 and within the tubular body 70 there are proximal and distal internal stents 76 and 78 respectively and at least one external stent 80 intermediate the proximal distal ends. A fenestration is provided at the distal end 72 of the stent graft 68. In this embodiment the fenestration 82 is in the form of a scallop extending from the distal end 72 of the stent graft 68. The fenestration 82 is aligned with the struts 84 and 86 of the distal internal self expanding zig zag stent 78 so that the sides of the fenestration 90 can be stitched by stitching 92 to the struts 84 and 86 along at least part of their length.

Radiopaque or MRI opaque markers 94 are provided each side of the fenestration another marker 96 is provided at the base of the fenestration to enable visualisation of the fenestration to an accurate position with respect to a branch vessel such as a coeliac artery.

- 15 -

Once again, it will be noted that when the stent graft 68 is compressed for deployment within a delivery device the fenestration 82 will close up but upon release the fenestration will open to provide access to the branch artery.

Figure 13A shows an alternative arrangement of a scalloped fenestration. In this embodiment the struts 93 and 95 of a zig-zag stent 97 are bent so that a more U-shaped fenestration 98 can be formed in the stent graft 99.

Figure 14 shows an alternative embodiment of a stent graft with a scalloped fenestration and Figure 15 shows a detailed internal view of the scalloped fenestration of Figure 14.

In Figure 14 the stent graft 100 comprises a tubular body of graft material 102 with a lumen therethrough. The distal end 104 of the stent graft has distally extending exposed stent 106 and within the tubular body 102 there are proximal and distal internal stents 108 and 110 respectively and at least one external stent 80 intermediate the proximal distal ends. A fenestration is provided at the distal end 104 of the stent graft 100. In this embodiment the fenestration 114 is in the form of a scallop extending from the distal end 104 of the stent graft 100. The fenestration 114 is aligned with spaced apart struts 116 and 118 of the distal internal self expanding zig zag stent 110 so that the sides of the fenestration 114 can be stitched by stitching 120 to the struts 116 and 118 along at least part of their length. A zig-zag portion 122 of the distal internal self expanding zig zag stent 110 extends uncovered through the fenestration and suture 124 joins a bend of the distally extending exposed stent 106 to a bend of the distal internal self expanding zig zag stent 110.

As can be seen in Figure 15 an arch of resilient wire 130 is stitched around the periphery 132 of the scalloped fenestration. The wire 130 has a loop 134 formed at each end of it so that no sharp end of the wire is provided which could damage the wall of a vessel into which the stent graft is deployed. Because the wire or other material from which the U-shaped reinforcement 130 is resilient the fenestration will close up when the stent graft is in a contracted state for deployment into a bodily lumen such as the aorta and when released will open up to enable blood flow through the fenestration to a branch vessel while at the same time ensuring

- 16 -

that the periphery 132 of the scalloped fenestration engages against the wall of a vessel into which it is deployed and provides sealing.

The enlarged fenestration of this embodiment is illustrated as a double width as it takes in regions between two pairs of struts of the stent but may also be provided as a triple width. The enlarged fenestration enables a stent graft to be placed where there are several branch vessels in close proximity to each other which should not be occluded.

The scalloped fenestration shown in Figures 12 to 15 have been illustrated as being on the distal end of a stent graft but they may also be provided on the proximal end of a stent graft with or without the uncovered self expanding stent.

The use of a resilient reinforcement around the periphery of the fenestration provides a much more dimensionally stable aperture for the deployment of a leg or side arm extension. Particularly if using a balloon expandable stent as a leg or side arm extension is used the force of the balloon expansion will not tend to tear the graft material which may occur if no reinforcement was provided. The resiliency allows the fenestration to close off during contraction for deployment but to open up to a desired size and shape upon release in situ.

Throughout this specification various indications have been given as to the scope of this invention but the invention is not limited to any one of these but may reside in two or more of these combined together. The examples are given for illustration only and not for limitation.

Throughout this specification and the claims that follow unless the context requires otherwise, the words 'comprise' and 'include' and variations such as 'comprising' and 'including' will be understood to imply the inclusion of a stated integer or group of integers but not the exclusion of any other integer or group of integers.

- 17 -

Claims

1. A stent graft comprising a tubular wall and at least one fenestration in the tubular wall, characterized in that the at least one fenestration includes periphery and a resilient material around at least a portion of the periphery, whereby the
5 resilient material provides dimensional stability to the fenestration.
2. A stent graft as in Claim 1 characterized in that the resilient material is selected from at least one of nitinol, stainless steel and an elastomeric material and in a form selected from at least one of a ring, a spring, an expandable ring and a partial ring.
- 10 3. A stent graft as in Claim 1 characterized in that the fenestration is adjacent an end of the tubular wall and the fenestration is in the form of a scallop which is open at one side.
4. A stent graft as in Claim 3 characterized in that the resilient material around the periphery of the fenestration is in the form of a U-shape, whereby during
15 deployment assists with opening up of the fenestration so that a vessel behind the fenestration can be catheterized.
5. A stent graft as in Claim 1 characterized in that the fenestration is in the form of a scallop provided at least one of an distal and an proximal end of the tubular wall and wherein struts of self expanding stents provide resilient peripheral
20 reinforcement around at least a portion of the fenestration, whereby when the stent expands upon deployment, the struts spread apart thereby opening up the fenestration.
6. A stent graft as in Claim 1 characterized in that the resilient material around the periphery is in the form of a ring.
- 25 7. A stent graft as in Claim 6 characterized in that the ring includes at least two turns of wire.
8. A stent graft as in Claim 7 characterized in that terminal ends of the wire of the ring are provided with a loop, whereby the wire does not present a pointed end of wire which could damage a vessel.
- 30 9. A stent graft as in Claim 6 characterized in that the ring is a ring of a resilient material.

- 18 -

10. A stent graft having a tubular wall and at least one fenestration in the tubular wall, characterized in that the at least one fenestration includes a periphery and a ring of resilient material around the periphery, whereby the ring provides dimensional stability to the fenestration to assist with sealing.

5 11. A stent graft as in Claim 10 characterized in that the fenestration includes a tubular extension extending from the tubular wall and extending to the ring.

12. A stent graft as in Claim 11 characterized in that the tubular extension includes a self expanding stent.

10 13. A stent graft as in Claim 11 characterized in that the tubular extension includes at least one of an associated lining and a covering of a biocompatible graft material.

14. A stent graft comprising a tubular wall and at least one fenestration, characterized in that the at least one fenestration including a tubular extension, the tubular extension including a stent and extending from and in fluid communication
15 with the fenestration.

15. A stent graft as in Claim 14 characterized in that the tubular extension includes at least one of an associated lining and a covering of a biocompatible graft material.

16. A stent graft as in Claim 14 characterized in that the stent in the tubular
20 extension is a self expanding stent.

17. A stent graft as in Claim 14 characterized in that the stent is in the form of a Gianturco style zig zag Z stent.

18. A stent graft as in Claim 14 characterized in that the stent is a nitinol self
expanding stent.

25 19. A stent graft as in Claim 15 wherein the bio-compatible graft material is at least one of on the inside and the outside of the stent on the tubular extension.

20. A stent graft as in Claim 14 characterized in that the tubular extension is placed on a reduced diameter portion of the tubular wall, whereby the overall diameter of the tubular wall is not significantly affected.

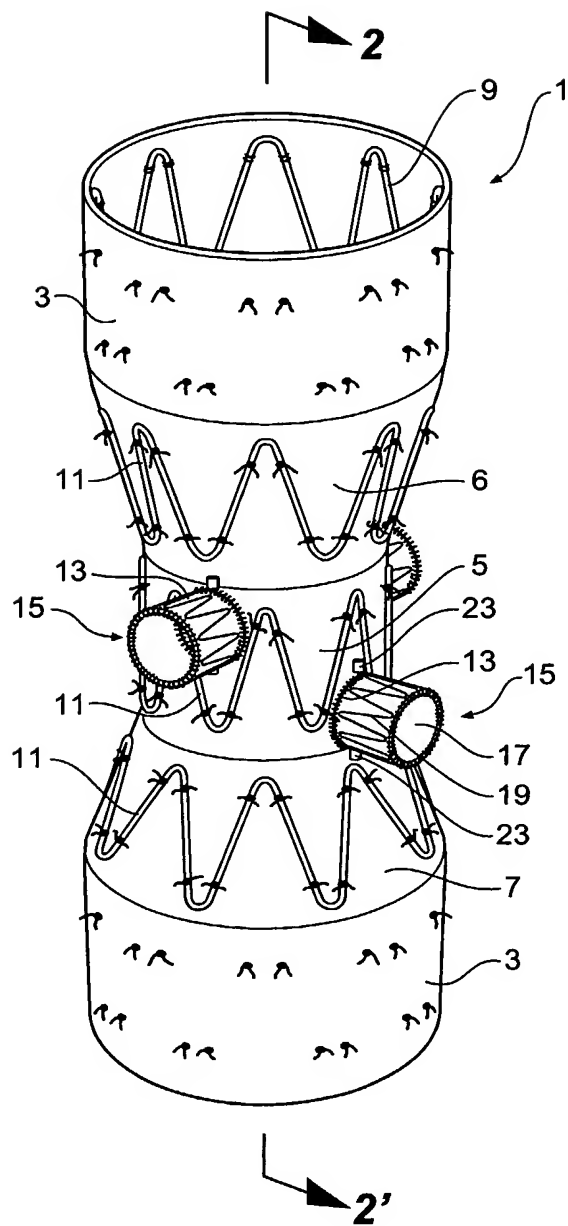


Fig 1

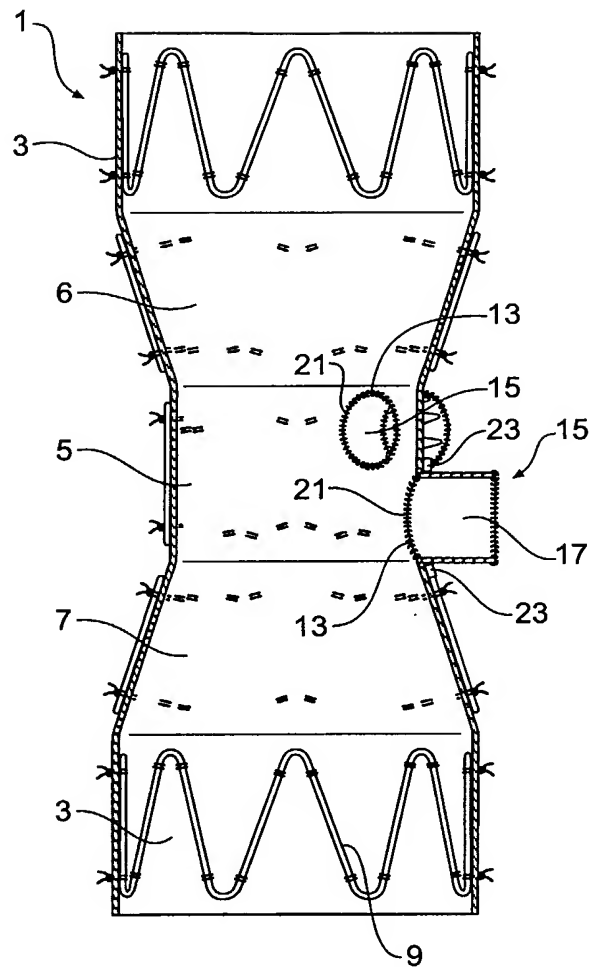


Fig 2

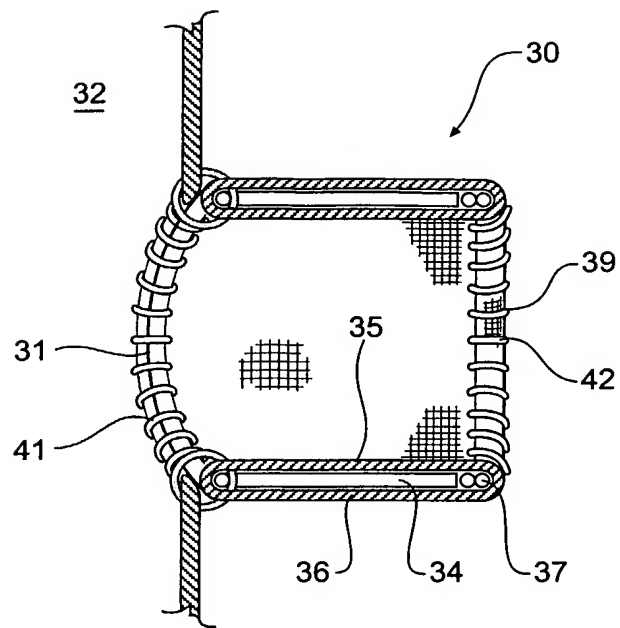


Fig 3

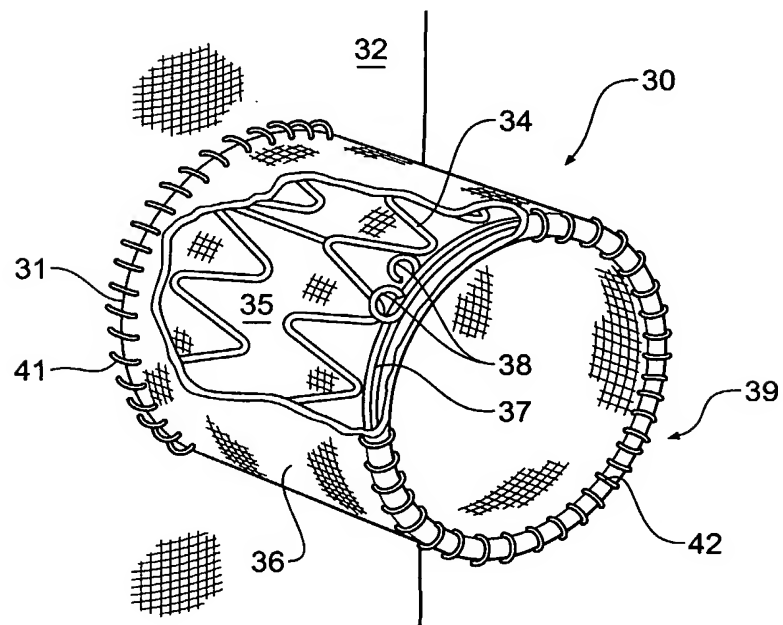


Fig 4

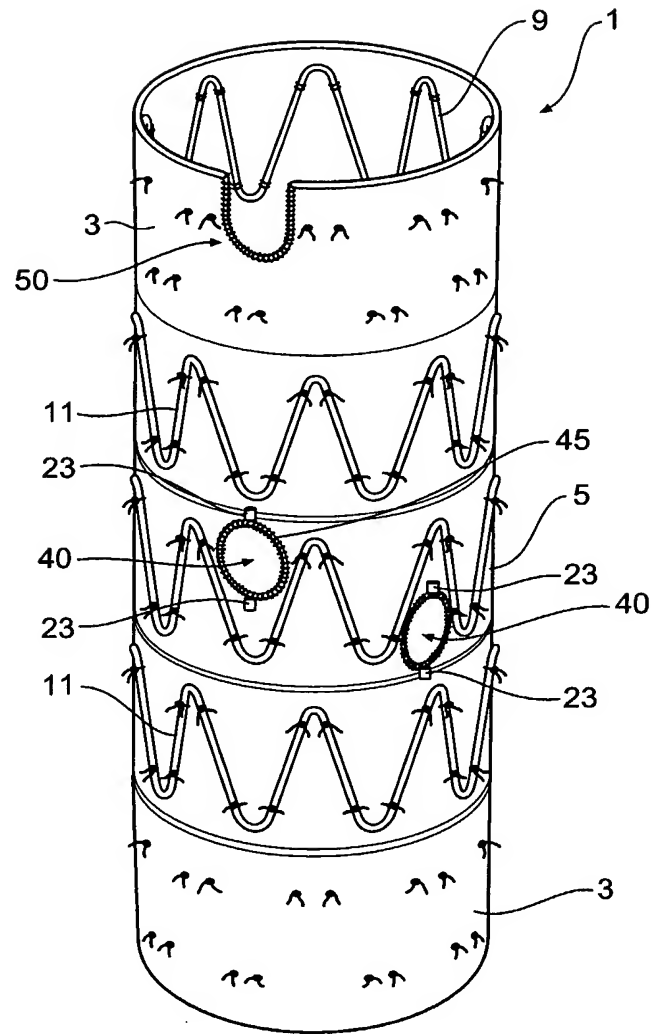


Fig 5

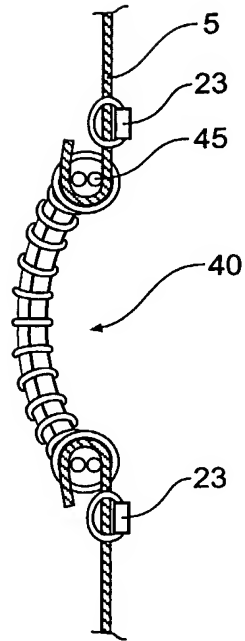


Fig 6

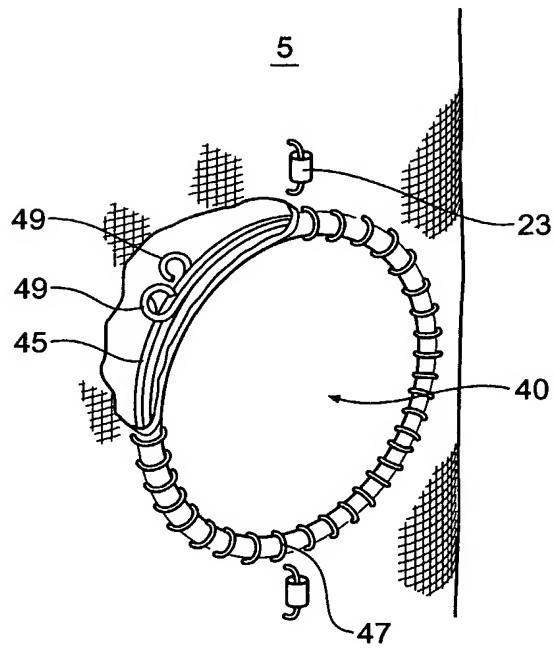


Fig 7

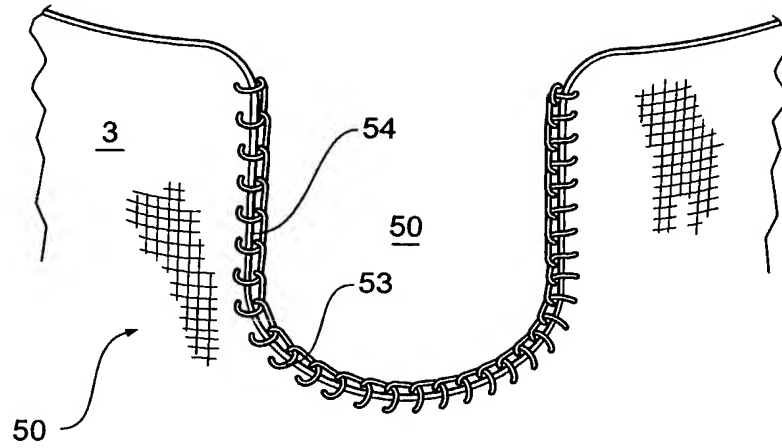


Fig 8

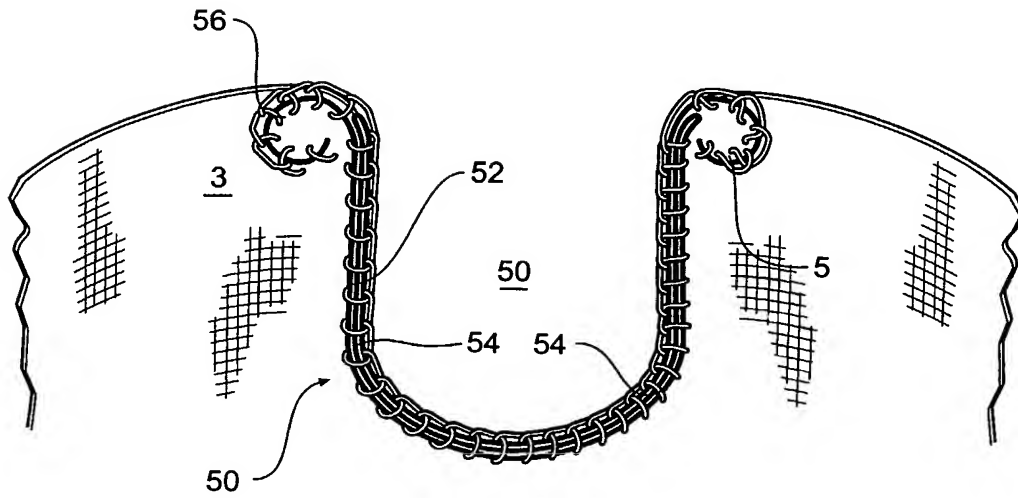
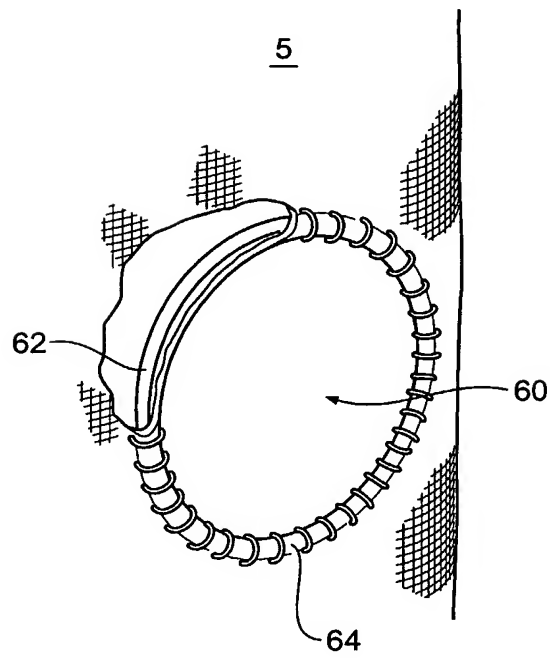
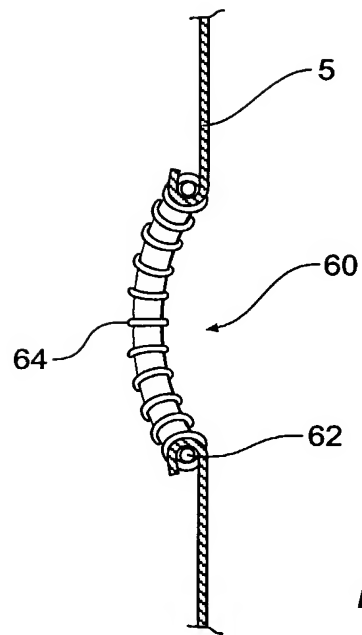


Fig 9



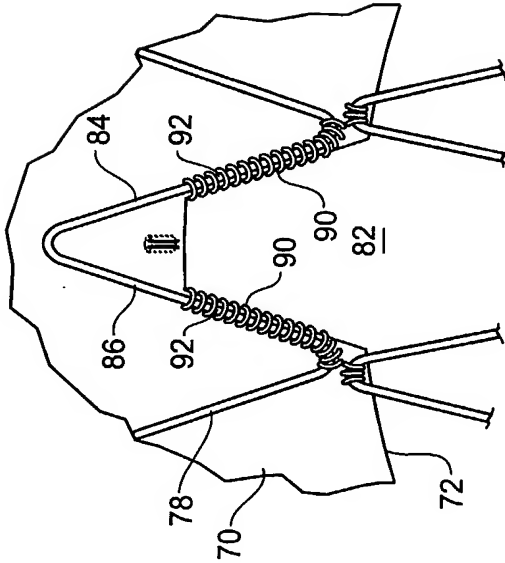


Fig 13

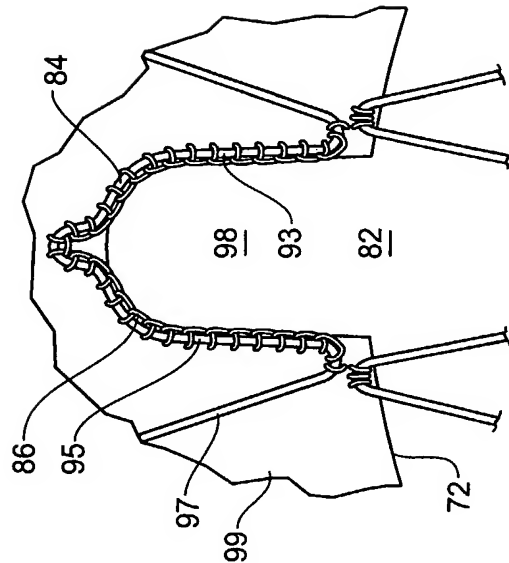


Fig 13A



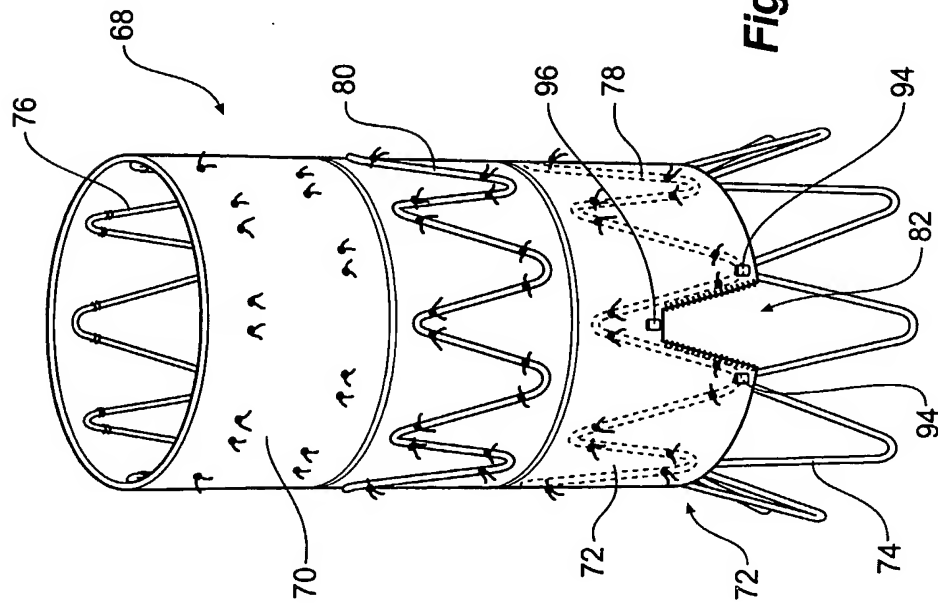


Fig 12

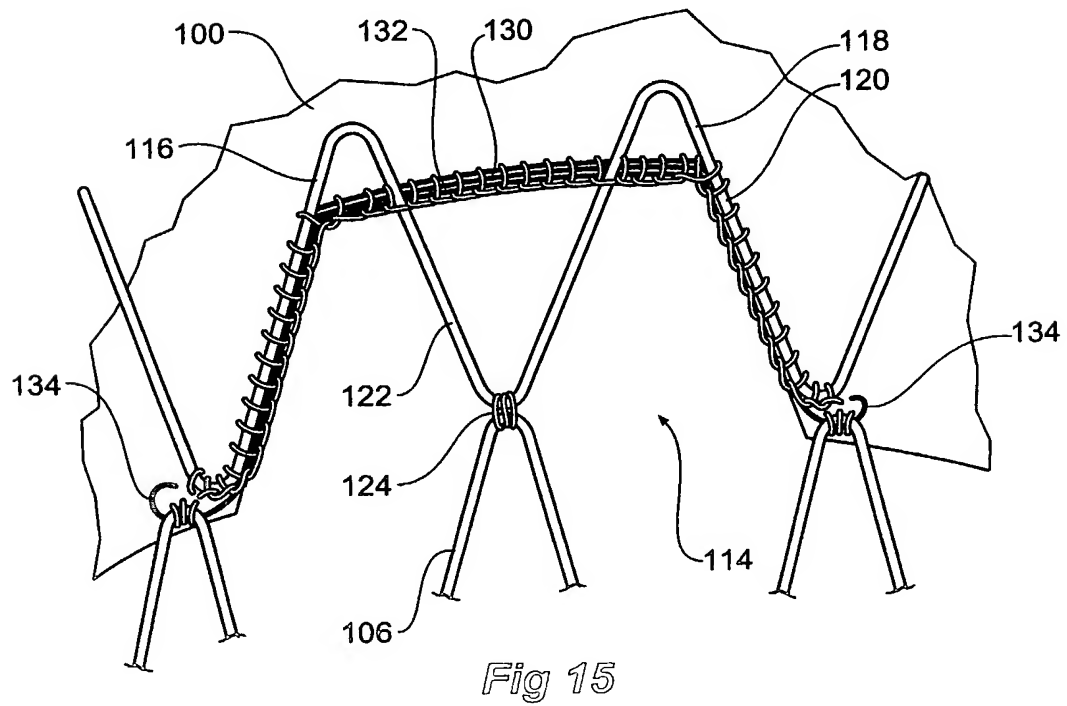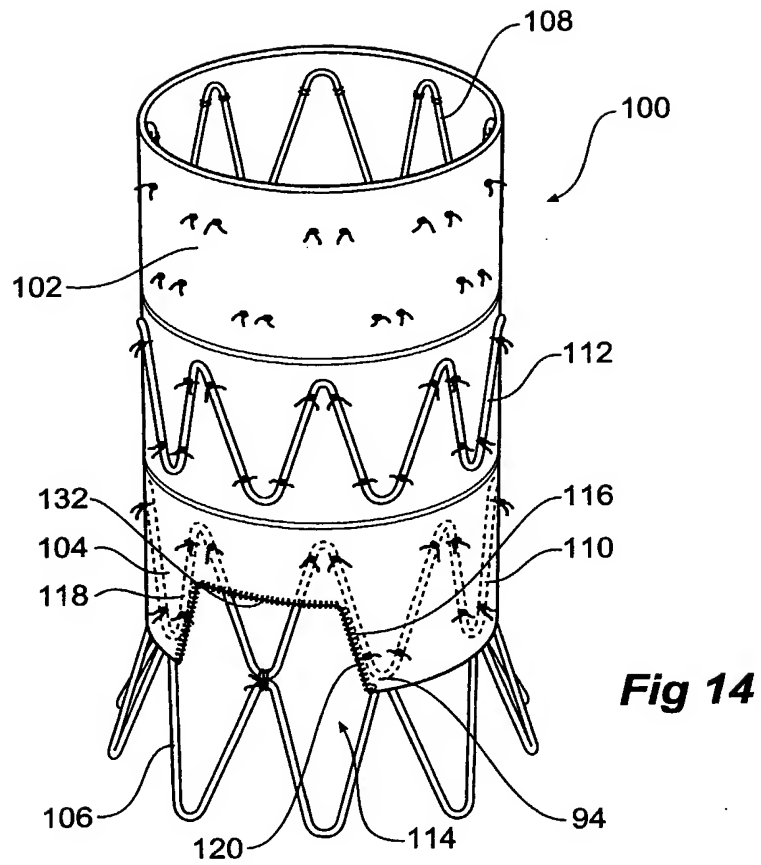

INTERNATIONAL SEARCH REPORT

International Application No
PCT/US2004/033568

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61F2/06

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 97/48350 A1 (SULZER VASCUTEK LTD) 24 December 1997 (1997-12-24) page 7, line 10 - page 11, line 32; figures 1-5	1-4, 6-8, 10
X	WO 03/082153 A2 (COOK INCORPORATED; WILLIAM A. COOK AUSTRALIA PTY. LTD; WILLIAM COOK EU) 9 October 2003 (2003-10-09) page 14, paragraph 5 - page 17, paragraph 2; figures 7-12	1, 2, 6, 9-19
X	US 5 961 548 A (SHMULEWITZ ET AL) 5 October 1999 (1999-10-05) column 4, line 23 - line 34; figure 3b ----- -/-	1, 2, 6, 9, 10, 14-16, 18-20

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *Z* document member of the same patent family

Date of the actual completion of the international search

25 January 2005

Date of mailing of the international search report

02/02/2005

Name and mailing address of the ISA

European Patent Office, P.B. 5618 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Skorovs, P

INTERNATIONAL SEARCH REPORT

Int'l Application No
PC 1/US2004/033568

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 02/067816 A1 (SCIMED LIFE SYSTEMS, INC) 6 September 2002 (2002-09-06) paragraph '0022! - paragraph '0048!; figures 1,2,7 -----	1,2,5,6, 9,10
X	US 2003/130719 A1 (MARTIN ERIC C) 10 July 2003 (2003-07-10) paragraph '0022! - paragraph '0048!; figures 1a,1c -----	1,2,6, 9-16, 18-20

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No
PCT/US2004/033568

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 9748350	A1	24-12-1997	DE 19624642 A1	22-01-1998
			DE 19633588 A1	26-02-1998
			AU 3182897 A	07-01-1998
			BR 9709867 A	11-01-2000
			CA 2258732 A1	24-12-1997
			CN 1226150 A	18-08-1999
			EP 0910309 A1	28-04-1999
			JP 2000512863 T	03-10-2000
			US 2002111665 A1	15-08-2002
			US 2002173837 A1	21-11-2002
			US 6740111 B1	25-05-2004
			US 2004199245 A1	07-10-2004
WO 03082153	A2	09-10-2003	CA 2474978 A1	09-10-2003
			EP 1487380 A2	22-12-2004
			US 2003199967 A1	23-10-2003
US 5961548	A	05-10-1999	NONE	
WO 02067816	A1	06-09-2002	WO 02067653 A2	06-09-2002
			WO 02067815 A1	06-09-2002
			US 2002193873 A1	19-12-2002
			US 2003097169 A1	22-05-2003
			US 2002173840 A1	21-11-2002
US 2003130719	A1	10-07-2003	NONE	